

# **INTEGRATION WITH DOSECONTROL<sup>®</sup>**

## **DOSIMETRY SOFTWARE – USER GUIDE**

# TABLE OF CONTENTS

<b>1</b>	<b>DESCRIPTION</b>	<b>3</b>
1.1	COMPLIANCE AND VALIDATION	3
1.2	DEFINITIONS	4
<b>2</b>	<b>GENERAL INSTRUCTIONS</b>	<b>5</b>
2.1	BEFORE YOU BEGIN	5
2.2	TURNING ON THIS FEATURE IN DOSECONTROL	5
2.3	DOSECONTROL SOFTWARE SETUP	7
<b>3</b>	<b>DATA IMPORT</b>	<b>10</b>
3.1	DESCRIPTION OF IMPORT TABLES	10
3.2	DESIGN SPECIFICATION - IMPORT TABLES	10
3.3	IMPORT PROCESS	16
3.4	IMPORT ERRORS	20
3.5	PRACTICAL EXAMPLE - IMPORT	22
3.6	HELPFUL REMINDERS	25
<b>4</b>	<b>DATA EXPORT</b>	<b>27</b>
4.1	DESCRIPTION OF EXPORT TABLES	27
4.2	DESIGN SPECIFICATION - EXPORT TABLES	28
4.3	EXPORT PROCESS	52

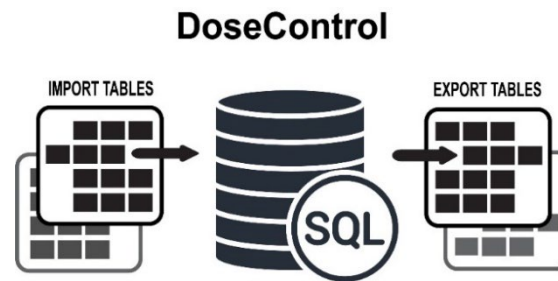
---

# 1 DESCRIPTION

This document provides instructions for how to import and export data into DoseControl® software from other systems (ERP, MES, QMS, SAP, NetSuite, PeopleSoft, etc.).

DoseControl software has a built-in structure to simplify and minimize costs to integrate with other systems - the standard Import and Export tables that are separate from the application database. If you upgrade to a newer version of DoseControl software, your integration remains intact.

Use a database professional within your own organization to push data into the SQL import tables and pull data from the SQL export tables.



Some integration examples:

- **Import process and product data into DoseControl software:** Make it easy for the operator to simply click and open the imported dosimetry report and begin measurements. Imported information reduces input errors.
  - Dosimeter IDs that were included in the irradiation process run.
  - Min and max dose specifications and correlation ratios.
  - Process-specific information such as Catalog Number, Product Description, etc.
- **Export process, product, and dosimeter measurement data from the DoseControl software:** Send dosimetry information to other systems for product release processes, process control, process data analysis, and the analysis of dosimetry related metrics.

## 1.1 Compliance And Validation

GEX has validated the functions of the tables and the population of data into these tables as a standard function of DoseControl. It is up to the user to validate the integration with these tables and the introduction of integrated data into and, if applicable, out of the software. This includes validation that the integrated data is both used and displayed within DoseControl, as applicable.

## 1.2 Definitions

**Dosimeter:** A device that, when irradiated, exhibits a quantifiable change in some property of the device that can be related to absorbed dose in a given material using appropriate analytical instrumentation and techniques. Dosimeters are packaged in a pouch, and a pouch may contain 1 dosimeter replicate (dosimeter A), 2 dosimeter replicates (dosimeter A and B), 3 dosimeter replicates (dosimeter A, B and C), or 4 dosimeter replicates.

**Dosimeter ID:** Unique ID for a dosimeter. DoseControl software enforces the rule that all Dosimeter IDs must be unique in the system.

**Absorbance (A):** The absorbance value measured by the spectrophotometer.  $A_o$  is the original (background) absorbance of an unirradiated dosimeter.  $A_i$  is the average Absorbance value for the measured absorbance.

**Thickness (T):** Dosimeter thickness value.

**Response (R) :** The Calculated Response value for the dosimeter  $(A_i - A_o / T)$  where  $A_i$  is the average absorbance of dosimeter replicates A through D. The software calculates Dose from Response.

**Dose:** A quantity of ionizing radiation energy imparted per unit mass of a specified material. The software calculates dose as  $\text{Response} = f(\text{Dose})$ .

**Adjusted Dose:** Also called “corrected dose”. The Adjusted Dose is the Dose multiplied by the correction factor of the Calibration.  $\text{Adjusted Dose} = \text{Dose} * \text{Correction Factor}$  (if any).

**Calibration (of a dosimetry system):** The Calibration is the dosimeter batch calibration (dosimetry system calibration), whose calibration curve coefficients are used by the software to calculate Dose. The Calibration is a set of operations that establish, under specified conditions, the relationship between values of quantities indicated by a measuring instrument or measuring system, or values represented by a material measure or a reference material, and the corresponding values realized by (dose) standards.

**Calibration curve:** Mathematical expression of the relation between dosimeter response and corresponding value of dose certified traceable to a national or international standard dose. The Calibration configuration stored in DoseControl software has a unique name and ID and has curve coefficients used to calculate the Dose for the specific dosimeter ID.

**Correction Factor:** A correction factor is used to make a linear correction factor for the Adjusted Dose calculation. Correction factor is typically not used and is a “1”. The Calibration configuration contains the Correction Factor field value.

**Pathway (Irradiation Pathway):** A “pathway” is the client’s facility, irradiator, or pathway within a given irradiator.

**Batch (Dosimeter Batch):** The dosimeter “batch” refers to a specific dosimeter film batch produced by the manufacturer. The batch has a consistent thickness and quality. GEX B3 dosimeters are identified by a 2 letter ID, for example batch ‘EA’ or ‘EB’.

**Instrument:** Refers to the spectrophotometer or reader used to measure dosimeter absorbance.

**Report:** Dosimetry report. Dosimeters are measured into a dosimetry report. The report contains information for the measurement session, such as the Calibration, Pathway, Batch, instrument (reader), etc. used to make the dosimeter measurements in the report. The report may have header fields with information specific to the client’s irradiation process. These fields are set up by the client and are specific their dosimetry process, such as process ID, process date/time, customer name, product name, process specification information, etc.

---

## 2 GENERAL INSTRUCTIONS

### 2.1 Before You Begin

The process of integrating with other systems will require the user to populate the DoseControl import tables with data from those systems. GEX has provided some suggested SQL scripts snippets, but customers may use any SQL methods they have experience with for extracting, transforming, transferring and loading data. To date, we have customers integrating with other SQL-based systems as well as Oracle-based systems. You may need some help and guidance along the way. Keep in mind that GEX is not in the custom integration business. However, we can, and will try our best to answer questions. We simply encourage this discussion well in advance of the need for assistance as we cannot predict our response times for initial configuration issues.

### 2.2 Turning on this Feature in DoseControl

#### 2.2.1 Enterprise License

2.2.1.1 Integration with DoseControl requires a specific module to be installed as part of your DoseControl Enterprise license.










#### 2.2.2 Setup "GEX Client Repository"

2.2.2.1 Login to DoseControl with global admin or System Admin user access. Go to the System (hammer/wrench icon) screen and expand the Application Settings.

2.2.2.2 Click the Integration Service<sup>1</sup> dropdown and select "GEX Client Repository" option. This will activate the Import/Export tables and allow you to integrate.

2.2.2.3 Do not enter a connection string in the 'Connection String' field unless you are instructed by GEX. Leave the field blank.

<sup>1</sup> In versions earlier than DoseControl v 2.0.0, Integration Service is called "Client Report Service".



DoseControl®Administrator | Logout

## CONFIGURATION

— APPLICATION SETTINGS

SETTING	SELECTED IMPLEMENTATION	CONNECTION STRING
Integration Service	<div>GE Client Repository</div>	
Sign in manager	<div>DoseControl user manager</div>	

SAVE CHANGES

+ DATABASE CONNECTION

+ STORAGE

© 2023 GEX Corporation. All Rights Reserved. DoseControl is a registered trademark of GEX Corporation.

2.0.0

## 2.3 DoseControl software setup

### 2.3.1 Use the EXTERNAL ID fields

- 2.3.1.1 Importing reports uses the EXTERNAL ID field values in DoseControl. See *Section 3.3 Import Process*.
- 2.3.1.2 Login to DoseControl as the global admin or Application Administrator. Go to the Setup (sprocket icon) screen. Setup all areas and ensure that the item's ID, Identifier or Name matches the EXTERNAL ID for all configurations in DoseControl software. See *Pathway Setup screenshot below*.

### 2.3.2 Setup the Pathway, Batch and Report Type as the “default”

- 2.3.2.1 DoseControl uses the active “default” Pathway, Batch and Report Type for importing reports. Example: If your integration processes use Pathway=Production Loop, Batch=EA, and Report Type=Production Report v2, these items must be active and the default in the software. See *Batches Setup screenshot below*.

### 2.3.3 Setup the Report Type header fields as “Is Editable”

- 2.3.3.1 In the Report Type configuration for each report header field, check the box titled “Is Editable”.
- 2.3.3.2 Avoid import errors by ensuring “Is Editable” value is checked for each required report header field. See *Report Types setup screenshots below*. **There is no supported way of removing a report from DoseControl or re-importing it - (see section 3.4.3 Import Errors).**





DoseControl®

← BACK

EDIT REPORT TYPE: Product Report v2

Report output options

Exporter Type: 

Ref Dose 1 Pack PDF

Open PDF file icon: 

Always present

Name: 

Product Report v2

Open Excel file icon: 

Always present

External ID: 

Product Report v2

FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	REQUIRED	IS EDITABLE	ADDITIONAL VALIDATION	DELETE
Specification ID	Text	Specification ID	Specification ID	Specification ID	2	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<div>Edit</div>	<div></div>
Min spec	Decimal	Min spec	Min spec	Min Dose	3	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
Max spec	Decimal	Max spec	Max spec	Max Dose	4	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
Ref to Min Ratio	Decimal	Ref to Min Ratio	Ref to Min	Ref to Min	5	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
Ref to Max Ratio	Decimal	Ref to Max Ratio	Ref to Max	Ref to Max	6	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
WO Number	Text	WO Number	WO Number		7	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
Process Date	Date	Process Date	Process ID		8	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		

SAVE

ADD FIELD

ADD REF DOSE FIELDS

ADD PRODUCT SPEC FIELDS

DoseControl®

← BACK

REPORT TYPES

☒ Hide Inactive Elements

REPORT TYPE	DEFAULT	IS ACTIVE	USE PRODUCT SPECS	COPY	COPY NAME	DELETE
E-beam Energy Test	<input type="radio"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<div>Copy</div>	<div></div>	
Dose Map	<input type="radio"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<div>Copy</div>	<div></div>	
Test Dosimetry Report	<input type="radio"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<div>Copy</div>	<div></div>	
Product Report v2	<input checked="" type="radio"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<div>Copy</div>	<div></div>	<div></div>

---

## 3 DATA IMPORT

### 3.1 Description of Import Tables

There are three (3) tables that are used for importing data into DoseControl and they are named:

- ***ImportReports***

This table is populated with data that tells DoseControl the key information needed to select a report type and dosimeter calibration to initiate a report with imported data. It is the equivalent to the create new reports screen.

- ***ImportReadings***

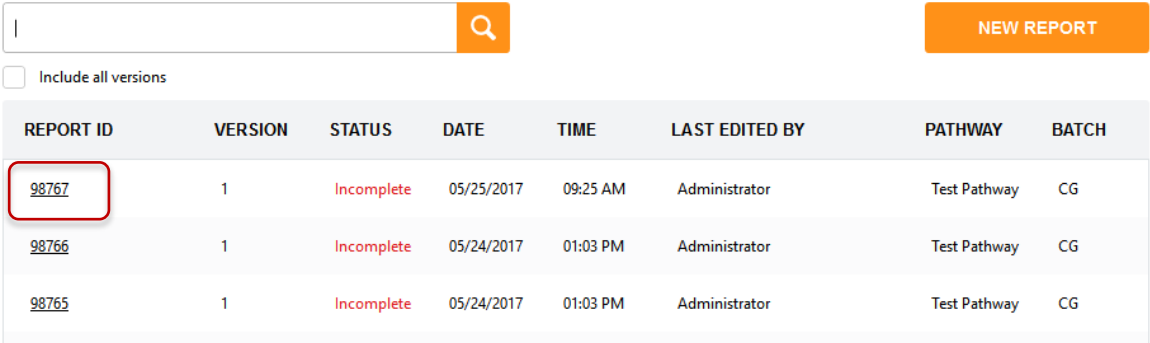
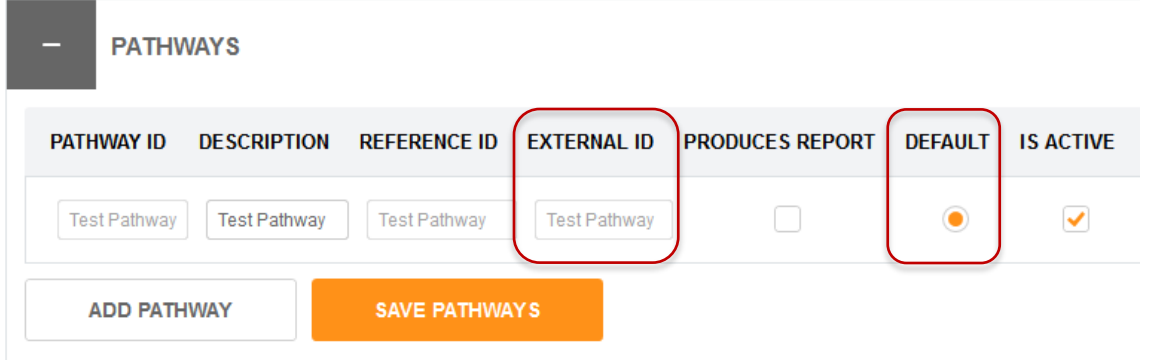
This table will be populated with the direct dosimeter information such as ID and position.

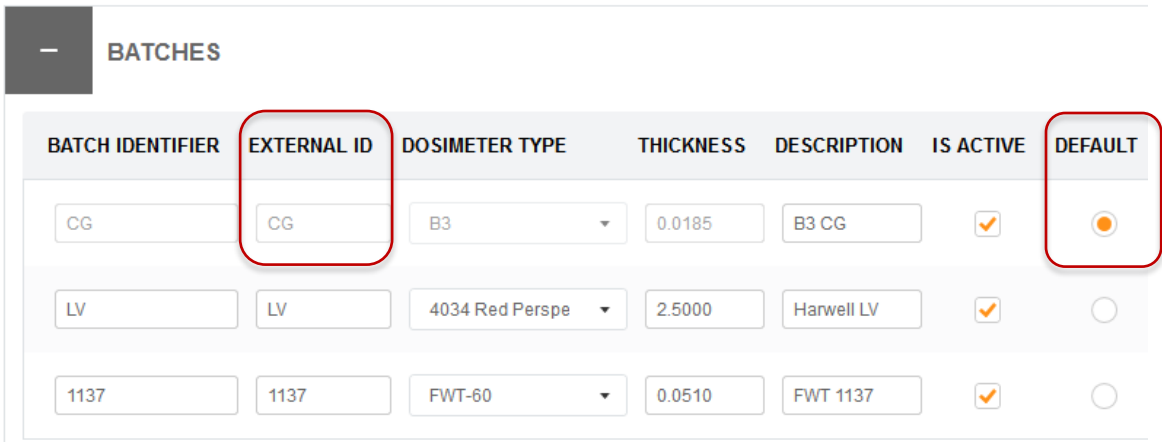
- ***ImportReportHeaderFieldValues***

This table must be populated with all product and process information that is required to be on-screen within any output that DoseControl produces (PDF, etc.).

### 3.2 Design Specification - Import Tables

Table Name: <b>ImportReports</b>		
<i>Column Name</i>	<i>Data Type</i>	<i>Notes</i>
Id	bigint	A database-generated unique ID.

ReportIdentifier	nvarchar(440)	<p><b>Report ID. Each Report ID must be unique in the software.</b> This value will be used as the key identifier of the report for users to select the DoseControl home screen; must be unique – duplicates will be treated as the same report. If you have a ‘process run ID’ that is the perfect value to insert here as the ‘ReportIdentifier’.</p> <p><b>SEARCH REPORTS</b></p> 
IrradiationPathwayId	nvarchar(440)	<p><b>Pathway ID.</b> Specifies the irradiation pathway the imported report should use. The value inserted in this column <u>must be identical with</u> the EXTERNAL ID field in ‘Pathways’ configuration in DoseControl (see image below). If no value is provided the default pathway will be used; use a static value in scripts to populate this column if the value is not part of your run data set.</p> 

BatchIdentifier	nvarchar(440)	<p>Specifies the batch the imported report should use. The value inserted in this column <u>must be identical with</u> the EXTERNAL ID field in 'Batches' configuration in DoseControl (see image below). If no value is provided the default batch will be used; use a static value in scripts to populate this column if the value is not part of your run data set.</p> 
-----------------	---------------	---

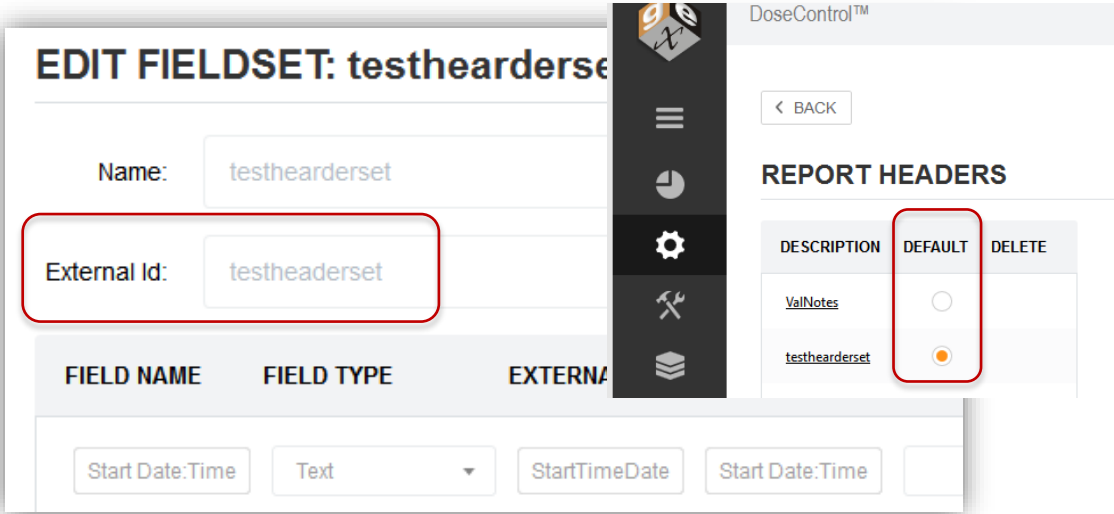
HeaderSetIdentifier	nvarchar (110)	<p>Specifies the header set that the newly imported report should use. The value inserted in this column <u>must be identical with</u> the EXTERNAL ID field in 'Report Headers' configuration in DoseControl (see image below). If the value is not provided the default header set will be used</p> 
CreatedDate	datetime	Allows to specify when the report was created. It is used for ordering reports before they are imported and is not displayed in the application.

Table Name: ImportReadings		
Column Name	Data Type	Notes
Id	bigint	Database-generated unique ID.
ImportReportId	bigint	The ID column value from the ImportReport table to which the reading belongs.

DosimeterIdentifier	nvarchar(max)	<b>Unique Dosimeter ID.</b> Value to identify the dosimeter packet (packet may contain more than one dosimeter); needs to be unique; can be a barcode value or any value used to uniquely identify each dosimeter processed through the irradiation system.
Position	nvarchar(max)	<b>Position identifier;</b> optional; identifies the position of the dosimeter in the 'tote' identified in 'TotelIdentifier' below.
TotelIdentifier	nvarchar(max)	<b>Tote identifier;</b> optional; may be a carrier, tray, etc., or it may be an identifier of a unique fixture used as the routine monitoring position.
Sequence	int	Value is used in determining the order of the readings inside of the report; optional; if no value is provided the database order will be used to sequence the DosimeterIdentifiers within DoseControl .

Table Name:

## ImportReportHeaderFieldValues

<i>Column Name</i>	<i>Data Type</i>	<i>Notes</i>
Id	bigint	Database-generated unique ID.
ImportReportId	bigint	The ID column value from the ImportReport table to which the header field belongs.

FieldIdentifier	nvarchar(200)	<p>A name used for identification of the field and <u>is not</u> the value from the run data. The value inserted in this column <u>must be identical with</u> the EXTERNAL ID field in the Header Set configured in 'Report Headers' and must match the report's HeaderSetIdentifier in the ImportReports table. In case no matching field is found, the field will be skipped, and no error will be returned.</p> <div><h3>EDIT FIELDSET: testheaderset</h3><div><div><div>Name:</div><div>testheaderset</div></div><div><div>External Id:</div><div>testheaderset</div></div></div><table><thead><tr><th>FIELD NAME</th><th>FIELD TYPE</th><th>EXTERNAL ID</th><th>LABEL</th><th>SPECIAL VALUE</th><th>SEQUENCE</th><th>R</th></tr></thead><tbody><tr><td>Start Date:Time</td><td>Text</td><td>StartTimeDate</td><td>Start Date:Time</td><td></td><td>1</td><td></td></tr><tr><td>End Date:Time</td><td>Text</td><td>EndTimeDate</td><td>End Date:Time</td><td></td><td>2</td><td></td></tr><tr><td>Batch Number</td><td>Text</td><td>BatchNumber</td><td>Batch Number</td><td></td><td>4</td><td></td></tr><tr><td>Scrap Quantity</td><td>Whole Number</td><td>ScrapQuantity</td><td>Scrap Quantity</td><td></td><td>5</td><td></td></tr><tr><td>Product Min Dose</td><td>Decimal Number</td><td></td><td>Min Dose Specification</td><td>Min Dose</td><td>6</td><td></td></tr><tr><td>Product Max Dose</td><td>Decimal Number</td><td></td><td>Max Dose Specification</td><td>Max Dose</td><td>7</td><td></td></tr></tbody></table></div>	FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	R	Start Date:Time	Text	StartTimeDate	Start Date:Time		1		End Date:Time	Text	EndTimeDate	End Date:Time		2		Batch Number	Text	BatchNumber	Batch Number		4		Scrap Quantity	Whole Number	ScrapQuantity	Scrap Quantity		5		Product Min Dose	Decimal Number		Min Dose Specification	Min Dose	6		Product Max Dose	Decimal Number		Max Dose Specification	Max Dose	7	
FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	R																																													
Start Date:Time	Text	StartTimeDate	Start Date:Time		1																																														
End Date:Time	Text	EndTimeDate	End Date:Time		2																																														
Batch Number	Text	BatchNumber	Batch Number		4																																														
Scrap Quantity	Whole Number	ScrapQuantity	Scrap Quantity		5																																														
Product Min Dose	Decimal Number		Min Dose Specification	Min Dose	6																																														
Product Max Dose	Decimal Number		Max Dose Specification	Max Dose	7																																														

Value	nvarchar(max)	The value assigned to a given field upon import. For example, if the Field Name is 'Product Description' then the value would be the actual description (e.g., "5mL Syringe 100pk").
-------	---------------	--

## 3.3 Import Process

Import tables serve as a queue for the reports to be imported from the application. Once a report is imported from the application it cannot be removed or imported again.

### 3.3.1 Ensure DoseControl is ready

3.3.1.1 See *Section 2.2 Turn on integration feature in DoseControl*, and *Section 2.3 Setup DoseControl software*.

### 3.3.2 Use a Single Transaction per Report

Each Report contains information from each of the three 3 Import tables (ImportReport, ImportReadings, ImportReportHeaderFieldValues) listed in section 3.2. GEX strongly suggests that you use one transaction to fill all three Import tables for each Report.

If you do not use a single transaction for each Report, a partial report import could occur causing errors. See section 3.4 Import Errors.

See the screenshot below for an example of the code used for a single transaction. (**IMPORTANT!** – *Your code will be different than the example below based on INSERT statements needed for your specific data sets.*)



```

USE [GEXApp]
GO

SET XACT_ABORT ON
BEGIN TRANSACTION;
    -- insert report
    DECLARE @importReportid BIGINT
    INSERT [dbo].[ImportReports] ([ReportIdentifier], [IrradiationPathwayId], [BatchIdentifier], [HeaderSetIdentifier],
[CreateDate]) VALUES (N'ABD', N'S8', N'CA', N'8B5E5B74-AEB9-4D36-9190-FB45F020DCE7', CAST(N'2017-01-01T00:00:00.000' AS datetime))
    set @importReportid = SCOPE_IDENTITY()
    --insert readings
    INSERT [dbo].[ImportReadings] ([ImportReportId], [DosimeterIdentifier], [Position], [ToteIdentifier], [Sequence]) VALUES
(@importReportid, N'ABC123', N'1', N'1', 1)
    INSERT [dbo].[ImportReadings] ([ImportReportId], [DosimeterIdentifier], [Position], [ToteIdentifier], [Sequence]) VALUES
(@importReportid, N'ABC124', N'2', N'2', NULL, 2)
    --insert header fields
    INSERT [dbo].[ImportReportHeaderFieldValues] ([ImportReportId], [FieldIdentifier], [Value]) VALUES (@importReportid,
N'ProductDescription', N'Some description')
    INSERT [dbo].[ImportReportHeaderFieldValues] ([ImportReportId], [FieldIdentifier], [Value]) VALUES (@importReportid,
N'TimerSetting', N'')
COMMIT
SET XACT_ABORT OFF

```

*Example script – the script writes data into the 3 Import tables (ImportReport, ImportReadings, ImportReportHeaderFieldValues) in a single transaction.*

### 3.3.3 The Report appears in the reports lists on the main screen

3.3.3.1 The DoseControl home screen lists the reports to be imported with a **status=New**. Until the report is imported, its status will be displayed as 'New' and no additional information (Date, Time, Edited By, Pathway, Batch) will be available.

## SEARCH REPORTS

Q

NEW REPORT

☐ Include all versions

REPORT ID	VERSION	STATUS	DATE	TIME	LAST EDITED BY	PATHWAY	BATCH
<a href="#">98767</a>	1	Incomplete	05/25/2017	09:25 AM	Administrator	Test Pathway	CG
<a href="#">98766</a>	1	Incomplete	05/24/2017	01:03 PM	Administrator	Test Pathway	CG
<a href="#">98765</a>	1	Incomplete	05/24/2017	01:03 PM	Administrator	Test Pathway	CG
<a href="#">98768</a>		New	N/A	N/A	N/A	N/A	N/A

3.3.3.2 The user must click the Report ID to import this report, and this action brings the Report information from the Import tables to the main application database. Once imported, the report will change its status to '**Incomplete**'. The Date and Time display when the report import occurred, Last Edited by is the user that imported the report, and the Pathway and Batch are associated with the report.

<a href="#">98768</a>	1	Incomplete	05/31/2017	05:10 PM	Administrator	Test Pathway	CG
-----------------------	---	------------	------------	----------	---------------	--------------	----

- 3.3.3.3 The user can click the Report ID to open the report. The software will display all the report header fields (the header fields where the value was provided in the import table will be filled in, while any other header fields will remain empty):

**DoseControl™**

### EDIT REPORT HEADER

**Report ID:** 98767 Version 1  
**Pathway ID:** Test Pathway  
**DSM Batch:** CG

Start Date:Time	April 14, 2017 11:01:01
End Date:Time	April 14, 2017 12:01:01
Batch Number	L654987
Scrap Quantity	3000
Min Dose Specification	5
Max Dose Specification	100
Ref to Min Ratio	0.5
Ref to Max Ratio	1
Catalog Number	CatNo321
Specification Code	SPEC4544
Product Description	Green Thing that Turns Yellow

*Example imported report's header field values.*

3.3.3.4 The user can proceed to measure dosimeters and complete the Report.

### 3.3.4 Managing the Import Table Data

You must manage the data in the import tables.

The records in the Import tables are not managed by DoseControl (or GEX) in any way. Once a report has been imported into DoseControl, its original records remain in the import tables but can be safely removed. The import table records will not be referenced or used in any way after they are imported into DoseControl.

## 3.4 Import Errors

### 3.4.1 Duplicate Dosimeter IDs

DoseControl requires Dosimeter IDs to be globally unique in the system. DoseControl software will not allow duplicate dosimeter IDs. If a user attempts to import (open) a newly imported report that contains duplicate dosimeter IDs, the user will be required to change the Dosimeter ID within the application using the screen below before proceeding:

**ACTION REQUIRED: Report 98768 contains duplicate Dosimeter IDs**

Below is a list of dosimeters used by different reports. In order to continue you must either rename or remove the ID.

ORIGINAL ID	NEW ID	IMPORT?
CG_1234567	<input type="text" value="CG_1234567"/>	<input checked="" type="checkbox"/>

Import

*Action Required prior to import of Report. Use can choose to change the dosimeter ID or not import the dosimeter.*

### ACTION REQUIRED: Report 98768 contains duplicate Dosimeter IDs

Below is a list of dosimeters used by different reports. In order to continue you must either rename or remove the ID.

ORIGINAL ID	NEW ID	IMPORT?
CG_1234567	CG_1234567R	<input checked="" type="checkbox"/>

Import

*User changes the dosimeter ID to a unique ID and is allowed to proceed importing the report.*

### 3.4.2 Wrong Batch/Pathway/Headerset

If a Batch, Pathway, or the Report Type (report header set) specified to DoseControl in the ImportReports table does not exist in the software dosimetry configuration, or is inactive in the software, or is not the “default” in the software, an error message will be displayed. This error can also occur if the application has not been configured yet by the administrator. See [section 3.3.1 Ensure DoseControl is Ready](#).

## Error

Importing the report failed. The expected batch with BatchIdentifier = CA2 was not found. Please contact your administrator.

OK

### 3.4.3 Imported Report Missing Necessary Values

If you make a report header field “Required” you also should make this field “Editable”. In the Report Types configuration, for each report header field, click the box titled “Is Editable”. Ensure this value is checked to allow the routine user to edit the imported values or fill them the report fields if they are imported as empty.

FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	REQUIRED	IS EDITABLE
Start Date:Time	Text	StartTimeDate	Start Date:Time		1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>

**IMPORTANT! There is no supported way of removing a report from DoseControl or re-importing it.** If you do not allow fields to be editable, a report experiencing this problem will not ever be allowed to be processed and will become an eternally incomplete record. We suggest creating another report with the same Report ID suffixed with a sequence number, and then manually import or send the data again on import with the suffixed ID.

### 3.4.4 Date Time values must be in valid regional format

Imported report header field date and time values must be in a valid format for the importing system (the importing PC’s regional settings).

For example, if these values are created on an English-US computer (10/26/2017 1:14:29 PM for example) and then imported on a computer that formats dates and times differently, say English-Austria that uses DD/MM/YYYY, then the import will fail.

## 3.5 Practical Example - Import

Below are examples of data in the import tables:

## ImportReports

GEX-LT09\SQLXP...bo.ImportReadings						
GEX-LT09\SQLXP...dbo.ImportReports						
GEX-LT09\SQLXP...HeaderFieldValues						
	Id	ReportIdentifier	IrradiationPath...	BatchIdentifier	HeaderSetIden...	CreatedDate
▶	2	98765	NULL	NULL	NULL	2017-04-12 15:37:17.710
	11	98766	NULL	NULL	NULL	2017-04-13 15:37:17.710
	12	98767	NULL	NULL	NULL	2017-04-14 15:37:17.710
	13	98768	NULL	NULL	NULL	2017-04-15 15:37:17.710
*	NULL	NULL	NULL	NULL	NULL	NULL

*ImportReports table example*

## ImportReadings

GEX-LT09\SQLXP...bo.ImportReadings						
GEX-LT09\SQLXP...dbo.ImportReports						
GEX-LT09\SQLXP...HeaderFieldValues						
	Id	ImportReportId	DosimeterIden...	Position	TotalIdentifier	Sequence
▶	1	2	CG_1234567	Ref	10	NULL
	3	2	CG_1234568	Ref	20	NULL
	4	2	CG_1234569	Ref	30	NULL
	5	11	CG_1234570	Ref	42	NULL
	6	11	CG_1234571	Ref	52	NULL
	7	11	CG_1234572	Ref	62	NULL
	8	12	CG_1234575	Ref	8	NULL
	9	12	CG_1234576	Ref	15	NULL
	10	13	CG_1234577	Ref	16	NULL
	11	13	CG_1234578	Ref	26	NULL
	12	13	CG_1234579	Ref	36	NULL
	13	13	CG_1234567	Ref	40	NULL
*	NULL	NULL	NULL	NULL	NULL	NULL

*ImportReadings table example*

## ImportHeaderFieldValues

GEX-LT09\SQLXP...bo.ImportReadings				
GEX-LT09\SQLXP...dbo.ImportReports				
GEX-LT09\SQLXP...HeaderFieldValues				
	Id	ImportReportId	FieldIdentifier	Value
	1	2	CatalogNumber	CatNo123456
	2	2	StartTimeDate	April 12, 2017 12:01:01
	3	2	EndTimeDate	April 12, 2017 13:01:01
	4	2	BatchNumber	Q1234567
	5	2	ScrapQuantity	0
	6	2	QuantityReceived	10000
	7	2	QuantityUnloaded	10000
	9	2	ProductDescripti...	Very Neat Device that Some Guy Invented and We Manufacture
	10	11	CatalogNumber	CatNo9999
	11	11	StartTimeDate	April 13, 2017 12:01:01
	12	11	EndTimeDate	April 13, 2017 14:01:01
	13	11	BatchNumber	Q33443344
	14	11	ScrapQuantity	1000
	15	11	QuantityReceived	300000
	17	11	QuantityUnloaded	299000
	18	11	ProductDescripti...	Very Different Device boxed for International
	19	12	CatalogNumber	CatNo321
	20	12	StartTimeDate	April 14, 2017 11:01:01
	21	12	EndTimeDate	April 14, 2017 12:01:01
	22	12	BatchNumber	L654987
	23	12	ScrapQuantity	3000
	24	12	QuantityReceived	30000
	25	12	QuantityUnloaded	27000
	26	12	ProductDescripti...	Green Thing that Turns Yellow
	27	13	CatalogNumber	CatNo123456
	32	13	StartDateTime	April 15, 2017 10:01:01
	36	13	EndDateTime	April 15, 2017 12:01:01
	37	13	BatchNumber	Q1234568
	38	13	ScrapQuantity	0
	39	13	QuantityReceived	200000
	40	13	QuantityUnloaded	200000
	41	13	ProductDescripti...	Very Neat Device that Some Guy Invented and We Manufacture
*	NULL	NULL	NULL	NULL

*ImportHeaderFieldValues table example*



Below is an example of the Report Type configuration and Product Specification configuration for the import data, as structured in the table above:

FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE
Catalog Number	Text	CatalogNumber	Catalog Number	Catalog Number	1
Product Description	Text	ProductDescription	Product Description	NULL	2
Batch Number	Text	BatchNumber	Batch Number	NULL	3
Quantity Received	Whole Number	Quantity Received	Quantity Received	NULL	4
Scrap Quantity	Whole Number	ScrapQuantity	Scrap Quantity	NULL	5
Quantity Unloaded	Whole Number	Quantity Unloaded	Quantity Unloaded	NULL	6
StartDate:Time	Date	StartTimeDate	StartDate:Time	NULL	7
EndDate:Time	Date	EndTimeDate	EndDate:Time	NULL	8
Specification Code	Text	NULL	Specification Code	Specification Id	9
Product Min Dose Spec	Decimal Number	NULL	Min Dose Specification	Min Dose	10
Product Max Dose Spec	Decimal Number	NULL	Max Dose Specification	Max Dose	11
Ref to Min Ratio	Decimal Number	NULL	Ref to Min Ratio	Ref to Min Ratio	12
Ref to Max Ratio	Decimal Number	NULL	Ref to Max Ratio	Ref to Max Ratio	13

## 3.6 Helpful Reminders

- 1) Match the EXTERNAL ID value with the appropriate Import table column name:
  - a. 'HeaderSetIdentifier' value inserted in this column must be identical with the EXTERNAL ID field in 'Report Type' configuration in DoseControl.
  - b. 'FieldIdentifier' value inserted in this column must be identical with the EXTERNAL ID field in the report header fields configured in 'Report Type' and must match the report's HeaderSetIdentifier in the ImportReports table. In case no matching field is found, the field will be skipped, and no error will be returned.
  - c. 'PathwayId' Value inserted in this column must be identical with the EXTERNAL ID field in 'Pathways' configuration in DoseControl.
  - d. 'BatchIdentifier' value inserted in this column must be identical with the EXTERNAL ID field in 'Batches' configuration in DoseControl.
  - e. All report header fields except 'CatalogNumber' that are imported into a report from the Product Specification Module do not require an EXTERNAL ID in header configuration.

2) Report Type setup:

- a. If you have a custom PDF report (provided by GEX), the Report Type's header 'Field Name' must be exact. GEX will give you the Field Names for the Report Type configuration.
- b. For the Report Type setup, you may use any text in the 'Label' column. The 'Label' is the on-screen displayed report fields and are modifiable before the report header is first used. Make sure you like the 'Label' name before importing reports.
- c. About report header field sequence – In the report type setup in section 3.5, the report header fields are listed in a sequence that was preferred by the customer. You may change the sequence of the report header fields before importing reports.
- d. Mark report header fields 'Required' if the data is required for that field before the user is allowed to 'Process Report' (i.e., export).
- e. **IMPORTANT!** Ensure any report header field marked 'Required' is also marked 'Is Editable' for all fields. See section 3.4.3 Import Errors.
- f. If you are using a Report Type setup with Product Specifications fields, follow the guidelines in the DoseControl User Guide (GEX Doc. 100-266):
  - [GEX Doc#100-266 DoseControl User Guide \(for DoseControl v. 1.5.2023.2.17000 and earlier\)](#)
  - *GEX Doc#100-266 DoseControl User Guide (for DoseControl v. 2.0.0)*

---

## 4 DATA EXPORT

### 4.1 Description of Export Tables

#### 4.1.1 On 'Process a Report': Exporting a Complete Report all dosimeter measurement information in the report

When the **user presses the 'Process Report' button**, the report's data is stored in four (4) tables, ExportReports, ExportComments, ExportDosimeters, ExportHeaderValues. These tables are separate from the master records in the application database.

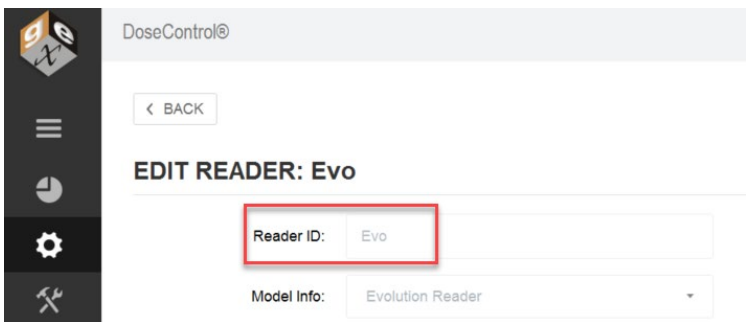
- **ExportReports:** DoseControl exports top level report information into this table such as the irradiation pathway and batch along with the key identifier, the Report ID, and its version number. The same Report ID can occur multiple times in this table but will be identifiable by the version number.
- **ExportComments:** DoseControl exports comments from reports into this table. Since the software has a versioning system for reports, different comments may be propagated into this table at different times depending on when a different version of a report is processed.
- **ExportDosimeters:** This table contains all the dosimetry details: absorbance, dose, thickness, and response of the dosimeter to the username that measured it, and the instrument serial number used for measurements.
- **ExportHeaderValues:** This table contains header field values that are associated with the report. Whatever fields are configured in the header will be posted here for retrieval. This includes header field whose values originate in the software and those that were imported into the software.

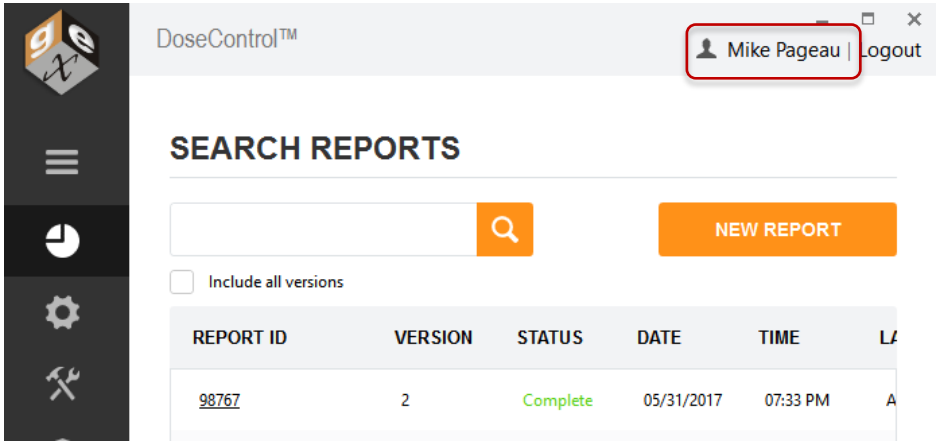
#### 4.1.2 On 'Measure a dosimeter': Exporting single dosimeter measurement information

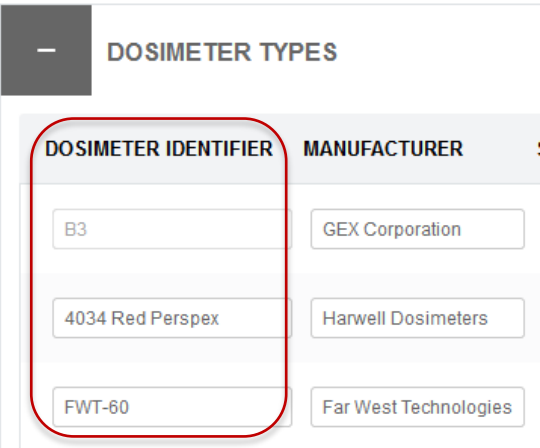
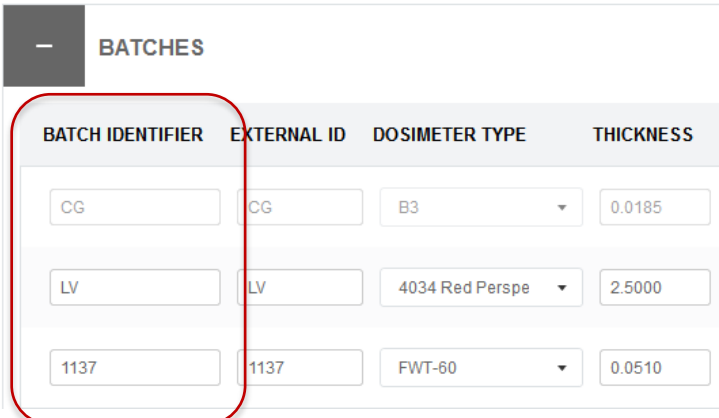
**When the user presses the 'Measure' button** on the measurement screen, the ExportMReadings table stores single measurement event values and the associated dosimetry information for that measurement event (Calibration, Batch, Reader, etc.) for a Dosimeter ID. This table is separate from the master records in the application database.

## 4.2 Design Specification - Export Tables

Table Name: ExportReports												
Column Name	Data Type	Notes										
Id	bigint	Database-generated unique ID.										
DosimetryReportId	nvarchar(440)	Report ID. This is identical to the 'ReportIdentifier' field that is explained in the imports section.										
Version	int	<div>Version of the report; the DosimeterReportId and Version pair is unique.</div> <div><div>SEARCH REPORTS</div><div><div><div></div></div><div><input type="checkbox"/> Include all versions</div><div><table><tr><th>REPORT ID</th><th>VERSION</th><th>STATUS</th><th>DATE</th><th>TIME</th></tr><tr><td><a href="#">98767</a></td><td>2</td><td>Complete</td><td>05/31/2017</td><td>07:33 PM</td></tr></table></div></div></div>	REPORT ID	VERSION	STATUS	DATE	TIME	<a href="#">98767</a>	2	Complete	05/31/2017	07:33 PM
REPORT ID	VERSION	STATUS	DATE	TIME								
<a href="#">98767</a>	2	Complete	05/31/2017	07:33 PM								
MeasurementInstrumentSn	nvarchar(440)	<div>Spectrophotometer or Reader's serial number</div> <div><div>Serial Number:</div><div>5A2T346001</div></div>										

MeasurementInstrumentId	nvarchar(440)	<p>Spectrophotometer or Reader's Spectrophotometer unique ID</p> 
MeasurementInstrumentWorkstationId	nvarchar(max)	Name of the PC to which the reader was assigned.
MeasurementInstrumentCalibrationDate	datetime	Spectrophotometer or Reader's last calibration date.
ReportCompleteDateTime	datetime	UTC formatted timestamp when the report was processed.

ReportUserName	nvarchar(max)	<p>Display name of the user processing the report.</p> 
ReportUserId	nvarchar(max)	<p>Username of the user logged into the PC that is processing the report.</p>

DosimeterType	nvarchar(max)	<p>The trade name or similar of the dosimeter used in the report.</p> 
DosimeterBatchId	nvarchar(max)	<p>Batch Identifier is the dosimeter batch ID.</p> 

NumberOfDosimeterReplicates	int	<p>'Absorbance count' of the calibration used in the report. This is how many dosimeters are used for each Dosimeter ID (e.g., 1 per pouch, 2 per pouch).</p> <p><b>EDIT CALIBRATION: 3199-CAcombo</b></p> <p>Display Name: <input type="text" value="CAL GEX B3 CG"/></p> <p>Calibration ID: <input type="text" value="3199-CAcombo"/></p> <p>External ID: <input type="text" value="00000000-0000-0000-0000-000000000000"/></p> <p>Pathway: <input type="text" value="Test Pathway"/></p> <p>Batch: <input type="text" value="CG"/></p> <p>Initial Avg Absorbance: <input type="text" value="0.000"/></p> <p>Reader ID: <input type="text" value="Device 1091"/></p> <p>Absorbance Count: <input type="text" value="1"/></p>
BatchCalibrationDate	datetime	<p>Calibration's Start Date:</p> <p>Coefficient C: <input type="text" value="-0.00351536308471458"/></p> <p>Coefficient D: <input type="text" value="0.00000893088474204544"/></p> <p>Coefficient E: <input type="text" value="0"/></p> <p>Start Date: <input type="text" value="5/22/2017"/></p> <p>End Date: <input type="text" value="5/22/2050"/></p> <p>Date Added: <input type="text" value="5/22/2017"/></p> <p>Wavelength: <input type="text" value="552"/></p>



CalibrationResponseFunctionId	nvarchar(max)	Calibration Identifier:  <b>EDIT CALIBRATION: 3199-CAcombo</b>  <div>             Display Name: <input type="text" value="CAL GEX B3 CG"/> </div> <div>             Calibration ID: <input type="text" value="3199-CAcombo"/> </div>
CalculatedRunMinimumDose	float	CalculatedRunMinimumDose is the report's overall Minimum adjusted dose (in kGy) of all measured dosimeters contained in the report. Adjusted dose = Dose * Ref:Min Ratio
CalculatedRunMaximumDose	float	CalculatedRunMaximumDose is the report's overall Maximum adjusted dose (in kGy) of all measured dosimeters contained in the report. Adjusted dose = Dose * Ref:Max Ratio

Table Name: <b>ExportComments</b>		
Column Name	Data Type	Notes
Id	bigint	Database-generated unique ID.


Comment	nvarchar(max)	Content of the comment from a particular version; includes both posted comments and skipped dosimeter information, if any. 
ReportVersion	int	Version of the Report ID the comment belongs to.
ExportReportId	bigint	Id column value of the ExportReport the comment belongs to.

Table Name: <b>ExportDosimeters</b>		
Column Name	Data Type	Notes
Id	bigint	Database-generated unique ID.

Identifier	nvarchar(max)	Dosimeter ID number: <div><div>— READINGS</div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
Position	nvarchar(max)	Dosimeter position information: <div><div>— READINGS</div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			

Tote	nvarchar(max)	Tote ID: <div><div>—</div><div>READINGS</div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
AbsorbanceValue	float	Average absorbance used for calculation the dose; can be 'null' for readings computed by statistical re-reads (not shown in image below): <div><div>—</div><div>READINGS</div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			

Thickness	float	<div>Average thickness of all absorbances. Depending on the configuration it can reflect manually entered thickness, measured thickness (if micrometer is configured), or the thickness value specified for the batch:</div> <div><div>—</div><div>READINGS</div><table><thead><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr></thead><tbody><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></tbody></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
Background	float	<div>Initial Average Absorbance of the calibration:</div> <div><div>EDIT CALIBRATION: 3199-CAcombo</div><div><div>Display Name:</div><div>CAL GEX B3 CG</div></div><div><div>Calibration ID:</div><div>3199-CAcombo</div></div><div><div>External ID:</div><div>00000000-</div></div></div>																																								

Response	float	Calculated response value $R=(A_i-A_o)/t$ <div><div>—</div><div>READINGS</div><table><thead><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr></thead><tbody><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></tbody></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
TotalNumberOfMeasurements	int	Total number of absorbance measurements for the Dosimeter. For example, if the dosimeter is measured once, value='1'. If the dosimeter is reread one time, value='2', etc.																																								
FinalDose	float	Adjusted dose for the dosimeter ID that is the final value after any rereads, according to user configured reread policy. <div><div>—</div><div>READINGS</div><table><thead><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr></thead><tbody><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></tbody></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
ExportReportId	bigint	ID column value of the ExportReport the dosimeter belongs to.																																								

DoselsUnderRange	bit (not null)	<p>Boolean value. True = reading is under the range of the calibration specified in the Calibration configuration. Otherwise, false.</p> <p><b>EDIT CALIBRATION: 3199-CAcombo</b></p> <hr/> <p>Display Name: <input type="text" value="CAL GEX B3 CG"/></p> <p>Calibration ID: <input type="text" value="3199-CAcombo"/></p> <p>External ID: <input type="text" value="00000000-0000-0000-0000-000000000000"/></p> <p>Pathway: <input type="text" value="Test Pathway"/></p> <p>Batch: <input type="text" value="CG"/></p> <p>Initial Avg Absorbance: <input type="text" value="0.000"/></p> <p>Reader ID: <input type="text" value="Device 1091"/></p> <p>Absorbance Count: <input type="text" value="1"/></p> <p>Dose Units: <input type="text" value="kGy"/></p> <p>Dose Range Min: <input type="text" value="1.4"/></p> <p>Dose Range Max: <input type="text" value="75.8"/></p>
------------------	----------------	--

DoselsOverRange	bit (Not null)	<p>Boolean value. True = reading is over the range of the calibration specified in the Calibration configuration. Otherwise, false.</p> <p><b>EDIT CALIBRATION: 3199-CAcombo</b></p> <p>Display Name: <input type="text" value="CAL GEX B3 CG"/></p> <p>Calibration ID: <input type="text" value="3199-CAcombo"/></p> <p>External ID: <input type="text" value="00000000-0000-0000-0000-000000000000"/></p> <p>Pathway: <input type="text" value="Test Pathway"/></p> <p>Batch: <input type="text" value="CG"/></p> <p>Initial Avg Absorbance: <input type="text" value="0.000"/></p> <p>Reader ID: <input type="text" value="Device 1091"/></p> <p>Absorbance Count: <input type="text" value="1"/></p> <p>Dose Units: <input type="text" value="kGy"/></p> <p>Dose Range Min: <input type="text" value="1.4"/></p> <p>Dose Range Max: <input type="text" value="75.8"/></p>
-----------------	----------------	---

Table Name: ExportHeaderValues		
Column Name	Data Type	Notes
Id	bigint	Database-generated unique ID.
ExportReportId	bigint	ID column value of the ExportReport the dosimeter belongs to.



ExternalIdentifier	nvarchar(max)	<div>EXTERNAL ID of the header field. This value is used during the import process to match imported fields with their appropriate field in configured report headers. Depending on configuration this value can be 'null':</div> <div>EDIT FIELDSET: testheaderset</div> <div><div><div>Name:</div><div>testheaderset</div></div><div><div>External Id:</div><div>testheaderset</div></div></div> <table><tr><th>FIELD NAME</th><th>FIELD TYPE</th><th>EXTERNAL ID</th><th>LABEL</th><th>SPECIAL VALUE</th><th>SEQUENCE</th><th>R</th></tr><tr><td>Start Date:Time</td><td>Text</td><td>StartTimeDate</td><td>Start Date:Time</td><td></td><td>1</td><td></td></tr><tr><td>End Date:Time</td><td>Text</td><td>EndTimeDate</td><td>End Date:Time</td><td></td><td>2</td><td></td></tr><tr><td>Batch Number</td><td>Text</td><td>BatchNumber</td><td>Batch Number</td><td></td><td>4</td><td></td></tr><tr><td>Scrap Quantity</td><td>Whole Numbe</td><td>ScrapQuantity</td><td>Scrap Quantity</td><td></td><td>5</td><td></td></tr><tr><td>Product Min Dos</td><td>Decimal Nurr</td><td></td><td>Min Dose Speci</td><td>Min Dose</td><td>6</td><td></td></tr><tr><td>Product Max Do:</td><td>Decimal Nurr</td><td></td><td>Max Dose Speci</td><td>Max Dose</td><td>7</td><td></td></tr></table>	FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	R	Start Date:Time	Text	StartTimeDate	Start Date:Time		1		End Date:Time	Text	EndTimeDate	End Date:Time		2		Batch Number	Text	BatchNumber	Batch Number		4		Scrap Quantity	Whole Numbe	ScrapQuantity	Scrap Quantity		5		Product Min Dos	Decimal Nurr		Min Dose Speci	Min Dose	6		Product Max Do:	Decimal Nurr		Max Dose Speci	Max Dose	7	
FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	R																																													
Start Date:Time	Text	StartTimeDate	Start Date:Time		1																																														
End Date:Time	Text	EndTimeDate	End Date:Time		2																																														
Batch Number	Text	BatchNumber	Batch Number		4																																														
Scrap Quantity	Whole Numbe	ScrapQuantity	Scrap Quantity		5																																														
Product Min Dos	Decimal Nurr		Min Dose Speci	Min Dose	6																																														
Product Max Do:	Decimal Nurr		Max Dose Speci	Max Dose	7																																														

FieldName	nvarchar(max)	<p>Name of the field. Value will always be provided:</p> <p><b>EDIT FIELDSET: testheaderset</b></p> <p>Name: <input type="text" value="testheaderset"/></p> <p>External Id: <input type="text" value="testheaderset"/></p> <table><thead><tr><th>FIELD NAME</th><th>FIELD TYPE</th><th>EXTERNAL ID</th><th>LABEL</th><th>SPECIAL VALUE</th><th>SEQUENCE</th><th>R</th></tr></thead><tbody><tr><td><input type="text" value="Start Date:Time"/></td><td><input type="text" value="Text"/></td><td><input type="text" value="StartTimeDate"/></td><td><input type="text" value="Start Date:Time"/></td><td><input type="text"/></td><td><input type="text" value="1"/></td><td></td></tr><tr><td><input type="text" value="End Date:Time"/></td><td><input type="text" value="Text"/></td><td><input type="text" value="EndTimeDate"/></td><td><input type="text" value="End Date:Time"/></td><td><input type="text"/></td><td><input type="text" value="2"/></td><td></td></tr><tr><td><input type="text" value="Batch Number"/></td><td><input type="text" value="Text"/></td><td><input type="text" value="BatchNumber"/></td><td><input type="text" value="Batch Number"/></td><td><input type="text"/></td><td><input type="text" value="4"/></td><td></td></tr><tr><td><input type="text" value="Scrap Quantity"/></td><td><input type="text" value="Whole Numbe"/></td><td><input type="text" value="ScrapQuantity"/></td><td><input type="text" value="Scrap Quantity"/></td><td><input type="text"/></td><td><input type="text" value="5"/></td><td></td></tr><tr><td><input type="text" value="Product Min Dos"/></td><td><input type="text" value="Decimal Num"/></td><td><input type="text"/></td><td><input type="text" value="Min Dose Speci"/></td><td><input type="text" value="Min Dose"/></td><td><input type="text" value="6"/></td><td></td></tr><tr><td><input type="text" value="Product Max Do"/></td><td><input type="text" value="Decimal Num"/></td><td><input type="text"/></td><td><input type="text" value="Max Dose Spec"/></td><td><input type="text" value="Max Dose"/></td><td><input type="text" value="7"/></td><td></td></tr></tbody></table>	FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	R	<input type="text" value="Start Date:Time"/>	<input type="text" value="Text"/>	<input type="text" value="StartTimeDate"/>	<input type="text" value="Start Date:Time"/>	<input type="text"/>	<input type="text" value="1"/>		<input type="text" value="End Date:Time"/>	<input type="text" value="Text"/>	<input type="text" value="EndTimeDate"/>	<input type="text" value="End Date:Time"/>	<input type="text"/>	<input type="text" value="2"/>		<input type="text" value="Batch Number"/>	<input type="text" value="Text"/>	<input type="text" value="BatchNumber"/>	<input type="text" value="Batch Number"/>	<input type="text"/>	<input type="text" value="4"/>		<input type="text" value="Scrap Quantity"/>	<input type="text" value="Whole Numbe"/>	<input type="text" value="ScrapQuantity"/>	<input type="text" value="Scrap Quantity"/>	<input type="text"/>	<input type="text" value="5"/>		<input type="text" value="Product Min Dos"/>	<input type="text" value="Decimal Num"/>	<input type="text"/>	<input type="text" value="Min Dose Speci"/>	<input type="text" value="Min Dose"/>	<input type="text" value="6"/>		<input type="text" value="Product Max Do"/>	<input type="text" value="Decimal Num"/>	<input type="text"/>	<input type="text" value="Max Dose Spec"/>	<input type="text" value="Max Dose"/>	<input type="text" value="7"/>	
FIELD NAME	FIELD TYPE	EXTERNAL ID	LABEL	SPECIAL VALUE	SEQUENCE	R																																													
<input type="text" value="Start Date:Time"/>	<input type="text" value="Text"/>	<input type="text" value="StartTimeDate"/>	<input type="text" value="Start Date:Time"/>	<input type="text"/>	<input type="text" value="1"/>																																														
<input type="text" value="End Date:Time"/>	<input type="text" value="Text"/>	<input type="text" value="EndTimeDate"/>	<input type="text" value="End Date:Time"/>	<input type="text"/>	<input type="text" value="2"/>																																														
<input type="text" value="Batch Number"/>	<input type="text" value="Text"/>	<input type="text" value="BatchNumber"/>	<input type="text" value="Batch Number"/>	<input type="text"/>	<input type="text" value="4"/>																																														
<input type="text" value="Scrap Quantity"/>	<input type="text" value="Whole Numbe"/>	<input type="text" value="ScrapQuantity"/>	<input type="text" value="Scrap Quantity"/>	<input type="text"/>	<input type="text" value="5"/>																																														
<input type="text" value="Product Min Dos"/>	<input type="text" value="Decimal Num"/>	<input type="text"/>	<input type="text" value="Min Dose Speci"/>	<input type="text" value="Min Dose"/>	<input type="text" value="6"/>																																														
<input type="text" value="Product Max Do"/>	<input type="text" value="Decimal Num"/>	<input type="text"/>	<input type="text" value="Max Dose Spec"/>	<input type="text" value="Max Dose"/>	<input type="text" value="7"/>																																														

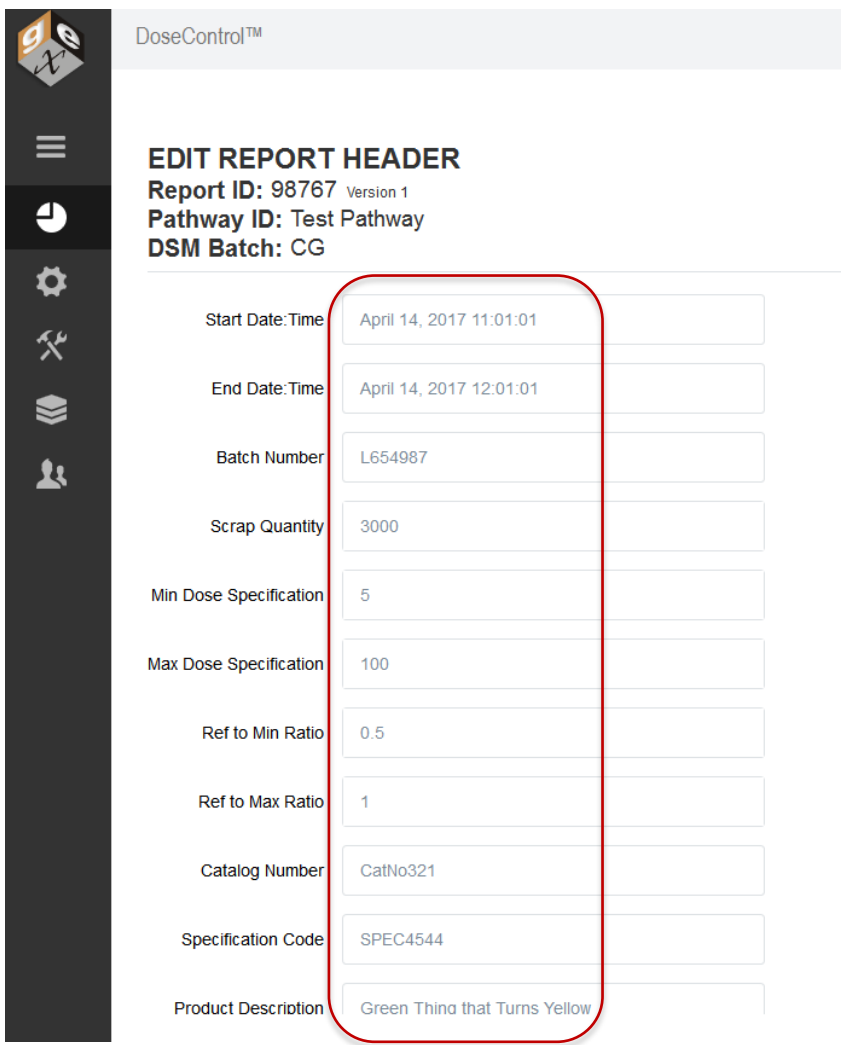
Value	nvarchar(max)	<p>The value of the header field.</p>  <p>DoseControl™</p> <h3>EDIT REPORT HEADER</h3> <p>Report ID: 98767 <small>Version 1</small>  Pathway ID: Test Pathway  DSM Batch: CG</p> <p>Start Date:Time April 14, 2017 11:01:01</p> <p>End Date:Time April 14, 2017 12:01:01</p> <p>Batch Number L654987</p> <p>Scrap Quantity 3000</p> <p>Min Dose Specification 5</p> <p>Max Dose Specification 100</p> <p>Ref to Min Ratio 0.5</p> <p>Ref to Max Ratio 1</p> <p>Catalog Number CatNo321</p> <p>Specification Code SPEC4544</p> <p>Product Description Green Thing that Turns Yellow</p>
-------	---------------	---

Table Name: ExportMReadings																																										
Column Name	Data Type	Notes																																								
Id	bigint	Database-generated unique ID.																																								
DSM_SN	nvarchar(max)	The unique number of the dosimeter. DoseControl cannot output two identical numbers unless all the configuration fields match. Specifically, there cannot be a duplicate ID from a different irradiation pathway, dosimeter batch, or measurement instrument. There should not be a need for the end-user to screen for duplicates ever existing in this field.																																								
CDose	float	<p>CDose is the “adjusted dose”. See Definitions. <math>CDose=MDose*Correction\ Factor</math>.</p> <div><div>—</div><div>READINGS</div><table><thead><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr></thead><tbody><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></tbody></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
Rev	Int (not null)	Rev is an Integer value indicating the dosimeter’s reading version . The dosimeter’s (DSM_SN) Rev value increases anytime that a measurement event, reread event, or skip measurement event occurs.																																								
Valid	Bit (not null)	Boolean value. True = reading is <u>within the range of the calibration specified in the Calibration configuration</u> . False = reading is outside the Calibration dose range.																																								
User	nvarchar(max)	The username of the user from application login. Varies depending on the login method configured and the individual user typology used.																																								

Name	nvarchar(max)	The full name of the user from application login. Varies depending on the login method configured and the individual user typology used but is designed for the user’s first and last name.																																								
Comment	nvarchar(max)	When a user skips a reading in the application a comment is required for that event. That comment will appear here, if applicable.																																								
Tote	nvarchar(max)	<div>From the field by same name in user interface of measure screen. The user can enter a Tote number, or you can use this field for another purpose.</div> <div><div><div>—</div><div>READINGS</div></div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
Pos	nvarchar(max)	<div>From the field by same name in user interface of measure screen. The user can enter a Position number, or you can use this field for another purpose.</div> <div><div><div>—</div><div>READINGS</div></div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			

Ao	float	<p>Original Absorbance (background absorbance) value of the dosimeter. The Ao is the “Initial Average Absorbance” value as configured in the Calibration used to determine dose for that dosimeter. May be NULL if not configured in the calibration.</p> <p><b>EDIT CALIBRATION: 3199-CAcombo</b></p> <p>Display Name: CAL GEX B3 CG</p> <p>Calibration ID: 3199-CAcombo</p> <p>External ID: 00000000-0000-0000-0000-00000000</p> <p>Pathway: Test Pathway</p> <p>Batch: CG</p> <p>Initial Avg Absorbance: 0.000</p> <p>Reader ID: Device 1091</p>
----	-------	---

AiA

float

Absorbance values for dosimeter replicate A from the measure screen for that dosimeter ID. If the Calibration used is configured with a 1, 2, 3 or 4 for “Absorbance Count”, the AiA value is the dosimeter absorbance measurement (the A measurement – the first and only dosimeter absorbance measurement).

The screenshot shows the DoseControl web application interface. At the top, there's a header with the DoseControl logo and a user menu showing 'Administrator | Logout'. Below the header, there's a navigation sidebar on the left with various icons. The main content area displays a report summary. Key information includes: Report ID: report 11.6.3 version 1, DSM Batch: EA, Pathway ID: Production Loop, and Reader Status: Ready. A table lists dosimeters with columns for #, ID, ABS, THICKNESS, and DOSE. The first row shows a dosimeter with ID EA\_640001, ABS 0.315, THICKNESS 0.0179 mm, and DOSE 17.1 kGy. To the right of the table, there's a 'MEASURE' section with input fields for Dosimeter ID, DSM Position, and Tote ID, and a 'MEASURE' button. Below this, the 'DOSE (kGy): 17.1' is displayed, and the 'A' value (Absorbance) is highlighted in a red box, showing 0.315. A 'REREAD' button is also present. At the bottom, it shows 'Readings: 1 of 1' and '0 Reader | Skip Reading'.

#	ID	ABS	THICKNESS	DOSE
1	EA_640001	0.315	0.0179 mm	17.1 kGy

MEASURE:

Dosimeter ID:

DSM Position:

Tote ID:

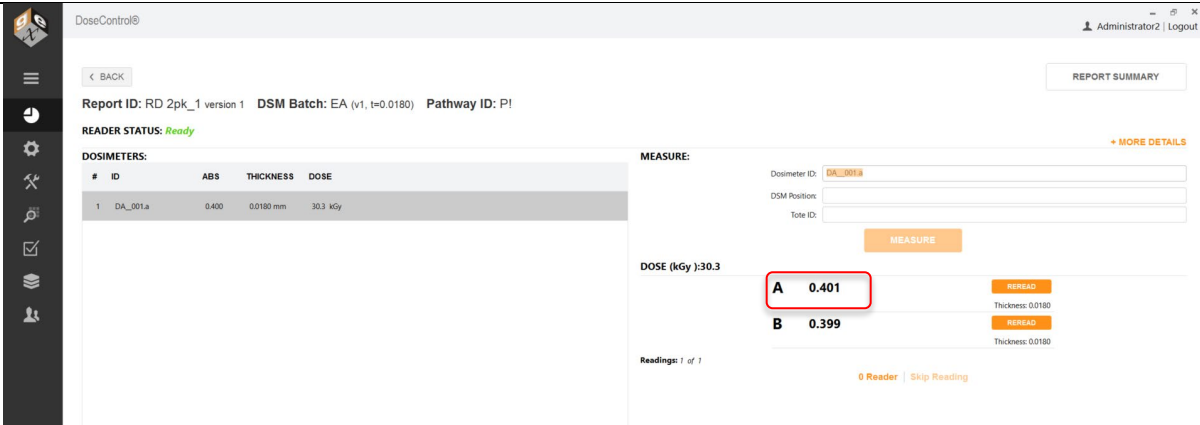
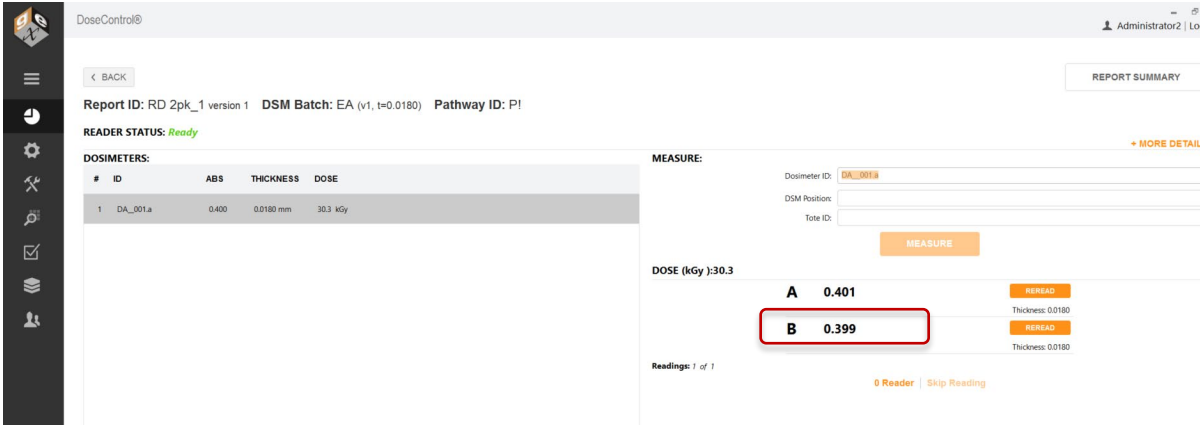
**DOSE (kGy): 17.1**

**A 0.315**

Readings: 1 of 1

0 Reader | Skip Reading

*Example report with AiA highlighted (1 dosimeter replicate)*

		 <p>Example report with AiA highlighted (2 dosimeter replicates)</p>
AiB	float	<p>Absorbance values for dosimeter replicate B from the measure screen for that dosimeter ID, if any. If the Calibration used is configured with a value of 2, 3 or 4 for “Absorbance Count”, the AiB value is the B dosimeter absorbance measurement (the B measurement – the second absorbance measurement in a series).</p> 



AiC	float	Absorbance values for dosimeter replicate C from the measure screen for that dosimeter ID, if any. If the Calibration used is configured with a value of 3 or 4 for “Absorbance Count”, the AiC value is the C dosimeter absorbance measurement (the C measurement – the third absorbance measurement in a series).																																								
AiD	float	Absorbance values for dosimeter replicate D from the measure screen for that dosimeter ID, if any. If the Calibration used is configured with a value of 4 for “Absorbance Count”, the AiD value is the D dosimeter absorbance measurement (the D measurement – the fourth absorbance measurement in a series).																																								
Tvalue	float	<div>Dosimeter thickness from the dosimeter batch that is used to determine dose for that dosimeter. Dosimeter batch thickness is configured in Batches in the application.</div> <div><div>—</div><div>READINGS</div><table><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></table></div>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
Resp	float	The calculated Response value for the dosimeter ( $A_i - A_o / T$ ) where $A_i$ is the average absorbance of dosimeter replicates A through D. (The Response is used to calculate MDose, (i.e., Dose))																																								

		<div><div>—</div><div>READINGS</div></div> <table><thead><tr><th>#</th><th>ID</th><th>TOTE</th><th>POSITION</th><th>ABSORBANCE</th><th>THICKNESS</th><th>RESPONSE</th><th>DOSE</th></tr></thead><tbody><tr><td>1</td><td>CG_1234577</td><td>16</td><td>Ref</td><td>0.250</td><td>0.0185 mm</td><td>13.514</td><td>16.4 kGy</td></tr><tr><td>2</td><td>CG_1234578</td><td>26</td><td>Ref</td><td>0.275</td><td>0.0185 mm</td><td>14.865</td><td>18.6 kGy</td></tr><tr><td>3</td><td>CG_1234579</td><td>36</td><td>Ref</td><td>0.285</td><td>0.0185 mm</td><td>15.405</td><td>19.5 kGy</td></tr><tr><td>4</td><td>CG_1234567R</td><td>40</td><td>Ref</td><td>0.286</td><td>0.0185 mm</td><td>15.459</td><td>19.5 kGy</td></tr></tbody></table>	#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE	1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy	2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy	3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy	4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy
#	ID	TOTE	POSITION	ABSORBANCE	THICKNESS	RESPONSE	DOSE																																			
1	CG_1234577	16	Ref	0.250	0.0185 mm	13.514	16.4 kGy																																			
2	CG_1234578	26	Ref	0.275	0.0185 mm	14.865	18.6 kGy																																			
3	CG_1234579	36	Ref	0.285	0.0185 mm	15.405	19.5 kGy																																			
4	CG_1234567R	40	Ref	0.286	0.0185 mm	15.459	19.5 kGy																																			
C_F	float	<p>Correction Factor. Correction Factor may be part of the Calibration configuration and is used to make a linear correction of the dose. See Definitions.</p> <div><div>Dose Range Min:</div><div>9.69</div></div> <div><div>Dose Range Max:</div><div>63.9</div></div> <div><div>Coefficient A:</div><div>2.51499931224723</div></div> <div><div>Coefficient B:</div><div>0.972967726465767</div></div> <div><div>Coefficient C:</div><div>-0.002689350169917</div></div> <div><div>Coefficient D:</div><div>0</div></div> <div><div>Coefficient E:</div><div>0</div></div> <div><div>Start Date:</div><div>5/24/2022</div><div>15</div></div> <div><div>End Date:</div><div>4/26/2025</div><div>15</div></div> <div><div>Date Added</div><div>4/26/2023</div><div>15</div></div> <div><div>Wavelength:</div><div>552</div></div> <div><div>Correction Factor:</div><div>1</div></div> <div><div>Is Active:</div><div><input type="checkbox"/></div></div> <div><div>Autogenerate dosimeter ids:</div><div><input type="checkbox"/></div></div> <div>SAVE CHANGES</div>																																								

MDose	float	MDose is “Dose”. Dose calculated from the Average Dosimeter Response. MDose is not visible on the screen.
Inst_SN	nvarchar(max)	The serial number of instrument (spectrophotometer or reader) used to acquire the absorbance readings for the dosimeter.
Inst_WL	int	The wavelength of measurement used to acquire the absorbance readings for the dosimeter.
Path	nvarchar(max)	The Pathway ID from application that the dosimeters were irradiated in. The pathway ID is configured in Pathways.
DSMbatch	nvarchar(max)	The dosimeter batch ID from the calibration configuration in the application.
DSMCal	nvarchar(max)	Calibration ID. The unique name of the Calibration stored in DoseControl used to calculate the doses for the specific dosimeter ID.
CreatedDate	Datetimeoffset(7)	Date and time of measurement event (measure, reread). UTC formatted timestamp.
IsStatisticalReread	Bit, null	Boolean value. True = the Absorbance value (AiA, AiB AiC or AiD) is a valid statistical reread absorbance value. False = the Absorbance value (AiA, AiB AiC or AiD) is the absorbance value for dosimeter replicate from the measure screen for that dosimeter ID. See “AiA, AiB AiC or AiD” above.
IsDoseUnderRange	Bit, not null	Boolean value. True = reading is under the range of the calibration specified in the Calibration configuration. Otherwise, false.
IsDoseOverRange	Bit, not null	Boolean value. True = reading is over the range of the calibration specified in the Calibration configuration. Otherwise, false.

## 4.3 Export Process

When reading from the export tables for integration purposes make sure that the SELECT queries specify the names of the columns instead of using the 'star' (SELECT \*) shorthand. This will prevent breaking changes to your integration scripts in the event GEX adds new columns to the export tables in future versions of DoseControl software.

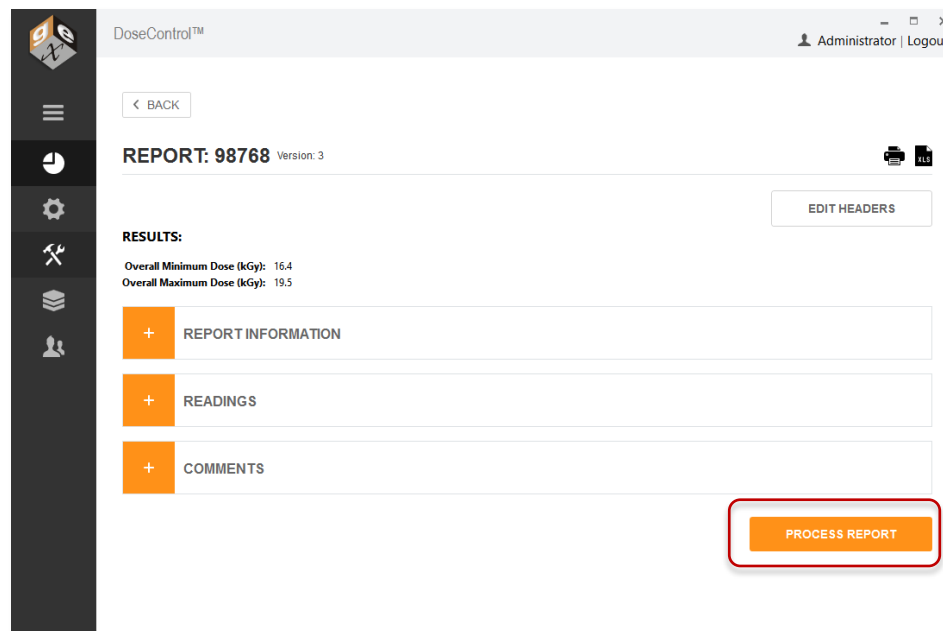
### 4.3.1 Managing the Export Table Data

The records in the Export tables are not managed in any way by DoseControl. DoseControl will push data to the export tables, and you must maintain the export tables and delete old data.

### 4.3.2 Export process for ExportReports, ExportDosimeters, ExportHeaderValues, ExportComments

The export process is triggered when the user clicks the **'Process Report'** button on the Report Summary screen. Report processing is confirmed by the user by clicking the "OK" button on the info message. (See screenshots below.)

A report can be processed anytime and may include missing (NULL) dosimeter readings. However, a report with no dosimeter readings cannot be processed. If the export fails, then the report processing will not complete. In the event of an export failure, contact GEX for assistance.



Info

Are you sure you want to process this report? This operation is irreversible.

OK

Cancel

### 4.3.3 Export process for ExportMReadings

Each time the **‘Measure’** button is pressed on the Measure screen, the data for that dosimeter is exported to the dbo.ExportMReadings table.

g e

≡

⌚

⚙

🔧

🔍

☑

📦

👤

DoseControl®

Administrator2 | Logou

< BACK

REPORT SUMMARY

Report ID: 518\_RD 1pack\_labels version 1

DSM Batch: EA (v2, t=0.0179)

Pathway ID: P!

READER STATUS: Ready

+ MORE DETAILS

DOSIMETERS:

#	ID	ABS	THICKNESS	DOSE
1	00000daV	0.391	0.0179 mm	21.1 kGy
2	0000089v	0.395	0.0179 mm	21.4 kGy
3	00000jrg	0.390	0.0179 mm	21.0 kGy

MEASURE:

Dosimeter ID: 00000daV

DSM Position:

Tote ID:

MEASURE

DOSE (kGy ):21.1

A 0.391

REREAD

Thickness: 0.0179

Readings: 1 of 3

0 Reader

Skip Reading

**REVISION HISTORY**

Date	Change Description	Revision
08/25/2018	Added ExportMReadings table specification. Edited Section 3.3 on exporting to coincide with changes to the latest release as of this date. ECO 70394.	D
01/13/2022	Improved the instructions in section 2.3 Import Process and changed the code block screenshot; this clarification ensures that the user's transaction will roll back and not make any changes to the database if there are errors during INSERTs. ECO 70598.	E
11/15/2023	<ul style="list-style-type: none"><li>-Added Definitions section to clarify meaning of words used in the document.</li><li>-Revised inconsistent use of words to align with the Definitions.</li><li>-Added section 2.3 DoseControl fields configuration.</li><li>-Revised Import Error section to include - Import tables must have valid Date Time imported data</li><li>-Revised Description of ExportMReadings table:<ul style="list-style-type: none"><li>•New column CreatedDate</li><li>•New column IsStatisticalReread</li><li>•New column IsDoseUnderRange</li><li>•New column IsDoseOverRange</li></ul></li><li>-Revised Description of ExportReports table:<ul style="list-style-type: none"><li>•Corrected design specification of ExportReports for columns CalculatedRunMinimumDose and CalculatedRunMaximumDose – these refer to adjusted dose min/max.</li></ul></li><li>-Revised import and export process section for clarity.</li></ul> ECO 70651	F